

See discussions, stats, and author profiles for this publication at: <https://www.researchgate.net/publication/305993325>

Abstract: A robust technique for detecting abdominal aortic calcification using dual energy x-ray absorptiometry

Conference Paper · June 2015

CITATIONS

0

READS

31

5 authors, including:



Karima Elmasri

University of Tripoli

3 PUBLICATIONS 8 CITATIONS

[SEE PROFILE](#)



Yulia Hicks

Cardiff University

92 PUBLICATIONS 781 CITATIONS

[SEE PROFILE](#)



Xin Yang

Cardiff University

8 PUBLICATIONS 25 CITATIONS

[SEE PROFILE](#)



Xianfang Sun

Cardiff University

125 PUBLICATIONS 1,892 CITATIONS

[SEE PROFILE](#)

Some of the authors of this publication are also working on these related projects:



3D face classification for medical application [View project](#)



3D Shape Classification [View project](#)

A Robust Technique for Detecting Abdominal Aortic Calcification Using Dual Energy X-Ray Absorptiometry

Karima M A Elmasri¹, Yulia Hicks¹, William D Evans^{1,3}, Xin Yang¹ and Xianfang Sun²

¹School of Engineering and ²School of Computer Science and Informatics, Cardiff University

³Medical Physics and Clinical Engineering, Cardiff and Vale University Health Board

Background:

Abdominal aortic calcification (AAC) is a marker of atherosclerosis and a predictor of subsequent vascular disease. To date, there has been little research into the automatic detection and quantification of AAC.

Methods:

In this study, lateral dual energy X-ray absorptiometry (DXA) scans are used to detect AAC; this is possible because of the anatomical position of the abdominal aorta anterior to the lumbar spine. The deformable shape modelling techniques active shape (ASM) and active appearance (AAM) models are used to model the calcified aorta and four vertebrae of the lumbar spine L1-L4.


Results:

ASM and AAM were trained and tested on 14 DXA images. The shape of both calcified aorta and four lumbar vertebrae were extracted automatically from the DXA scans using combined shape and appearance models.

Conclusion:

ASM and AAM were implemented successfully. The calcified aorta obtained from the DXA scans was segmented using this modelling technique. The next step is to develop a new automated method to quantify the calcification within the aorta.

All Wales Summer Meeting Medical Physics & Clinical Engineering ABSTRACTS

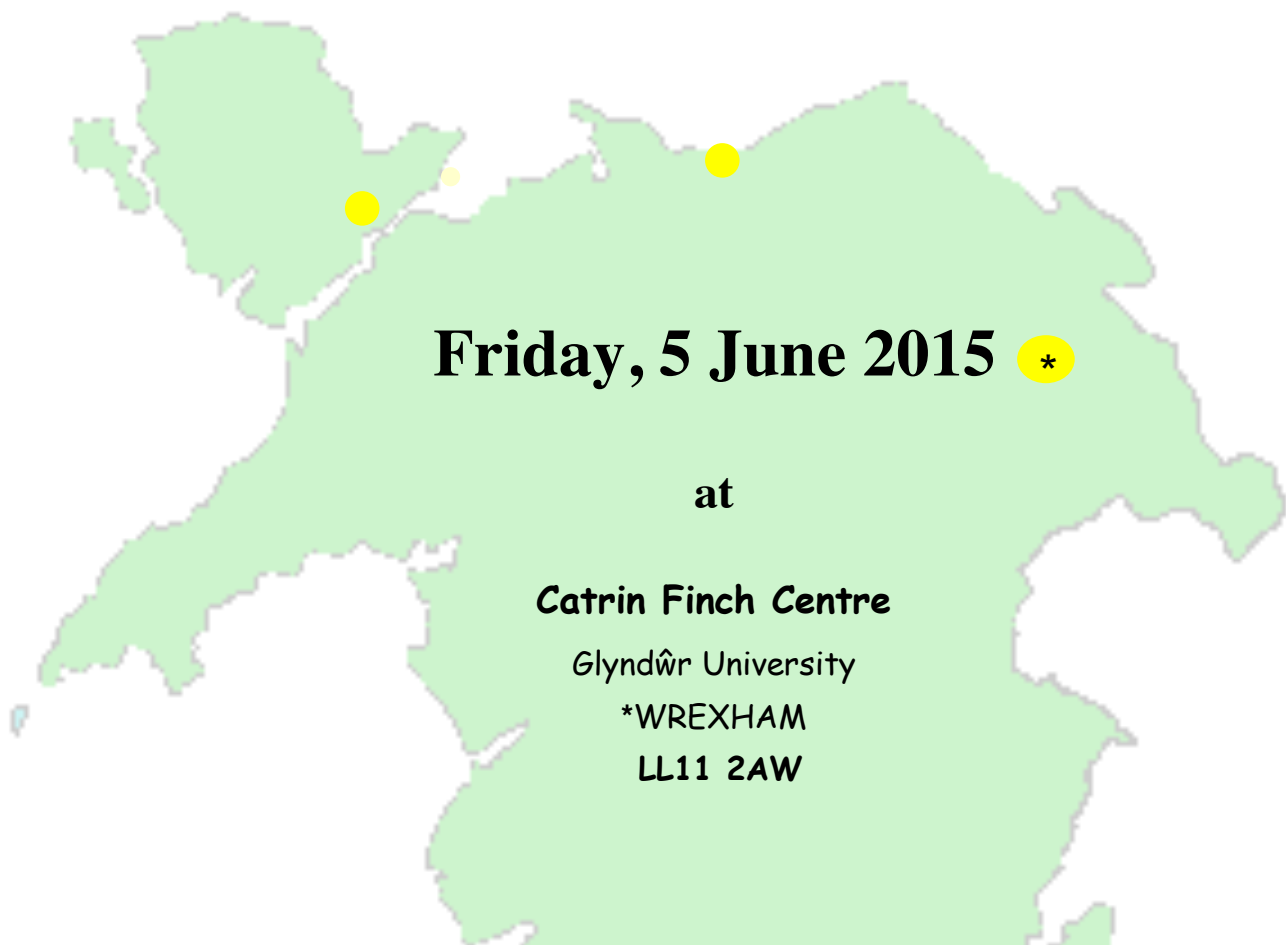

***Organised by
North Wales Medical Physics***